

INSTALLATION GUIDE USER MANUAL

TOP-CHECK TRANSFER

For TOP-CHECK FE-B and TOP-CHECK FN-B with firmware version 6.3 and up

Version 2.4 dated **2018-10**



LIST-MAGNETIK
Dipl.-Ing. Heinrich List GmbH
D-70771 Leinfelden-Echterdingen Max-Lang-Str. 56/2
Fon: + 49 (711) 903631-0 Fax: + 49 (711) 903631-10
Internet: <http://www.list-magnetik.de>
E-mail: info@list-magnetik.de



CONTENTS


TOP-CHECK TRANSFER (2018-10)

1. TOP-CHECK TRANSFER Application	2
2. Preparing Bluetooth Connection.....	3
A) Installation of the Bluetooth USB Dongle.....	3
B) Pairing TOP-CHECK.....	4
Detecting the COM-Port	6
3. Installing the Application.....	7
4. Functions	8
Step 1: Connect.....	8
Measuring Online	9
Read data from device	10
Output: File, Printer, Applications.....	11
Open Data File	12

1. TOP-CHECK TRANSFER APPLICATION

At www.list-magnetik.com in the „Download“ area you can obtain the free of charge application **TOP-CHECK TRANSFER** to transfer data from you TOP-CHECK device to a Windows PC or laptop.

With TOP-CHECK TRANSFER you can measure online, or read the device's memory, you can print the results or transfer them to various applications like Microsoft Word or Microsoft Excel.

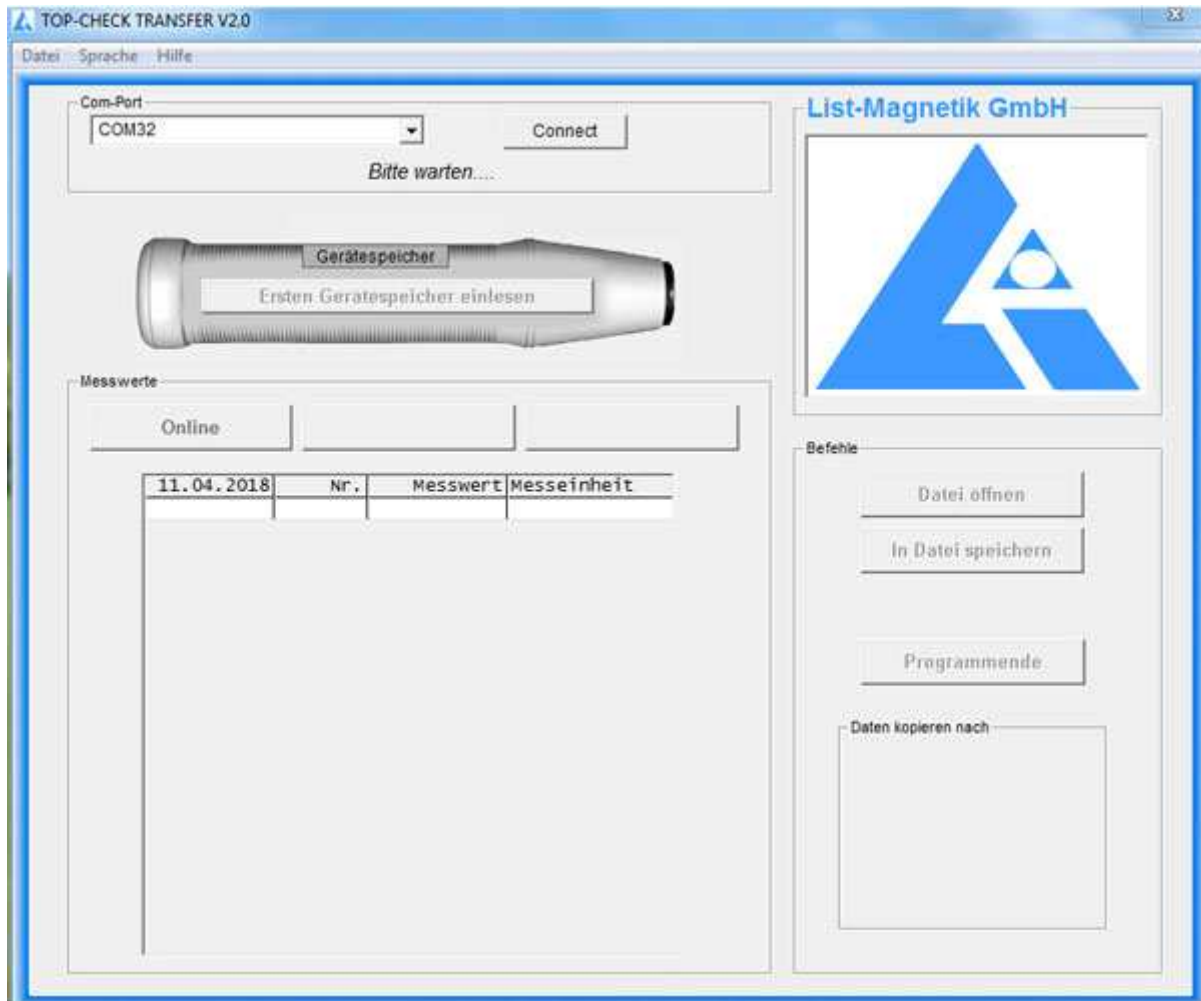

2. PREPARING BLUETOOTH CONNECTION

Does your PC / laptop have a built-in Bluetooth interface?

If yes, skip point 2a and continue at 2b.

A) INSTALLATION OF THE BLUETOOTH USB DONGLE



For TOP-CHECK FE-B and FN-B a Bluetooth dongle is included as shown.

The additional installation of a driver software can be used for communication setup between TOP-CHECK and a Windows PC. Please check first, if the connection between TOP-CHECK and your PC via Bluetooth works without software installation, only by inserting the Bluetooth dongle.

If you can't connect, perform the installation of the driver that can be obtained at

<http://www.list-magnetik.com/de/download>




under the heading "Software". The file is named BCM20702 _..., depending on the version of your Windows operating system. It is available for Windows XP, Win 7, Win 8 or Win 10.



B) PAIRING TOP-CHECK

Your TOP-CHECK device must be paired with the PC.

For this purpose, the coupling must be executed on both devices.

The function **SETUP / BLUETOOTH / ON** must be executed at the TOP-CHECK device, and afterwards a device search in the Bluetooth menu on the PC.

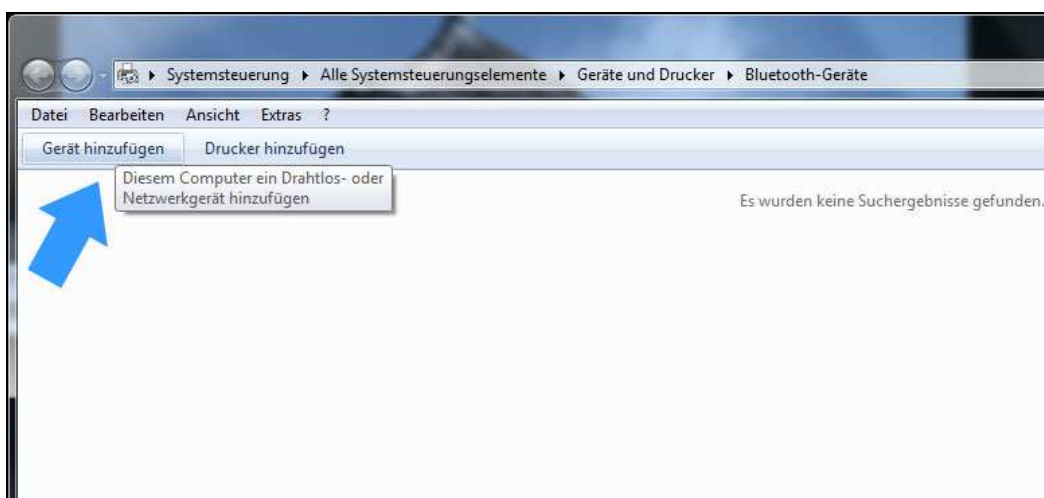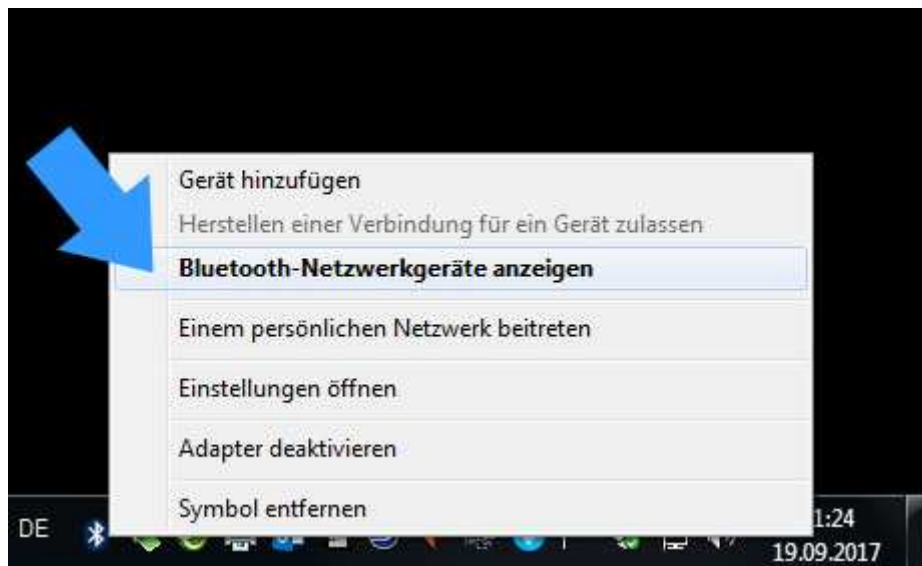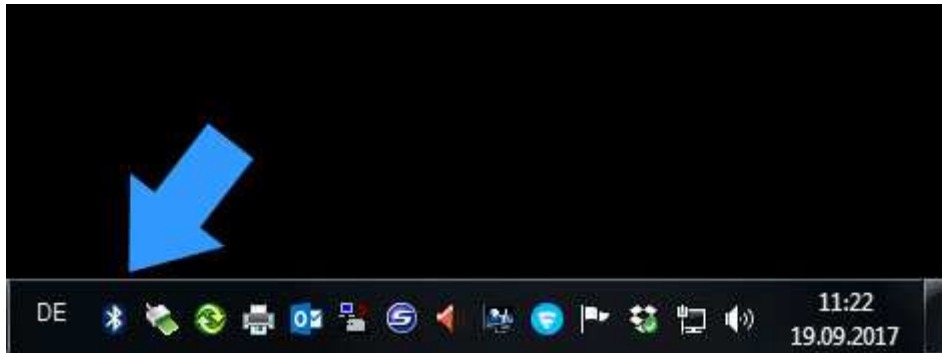


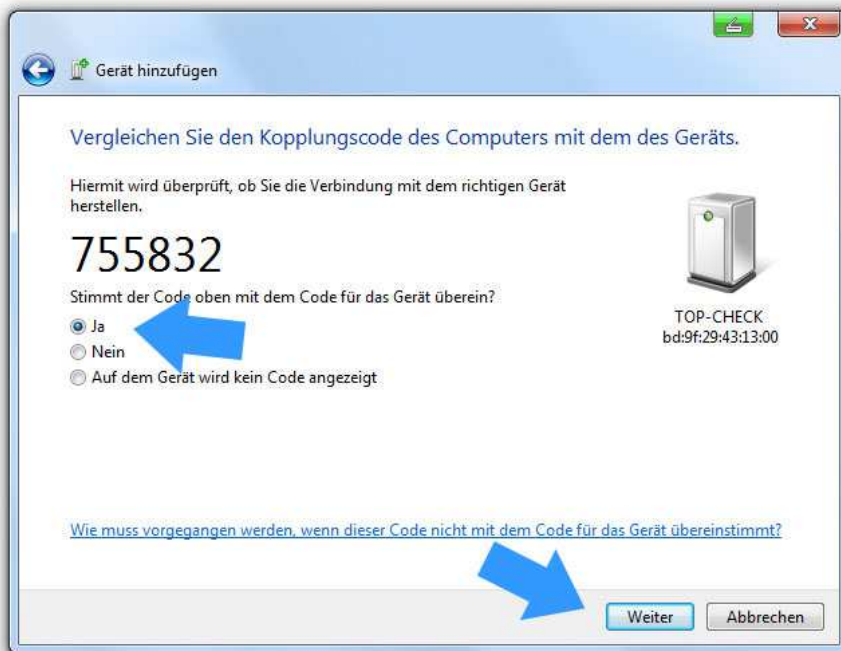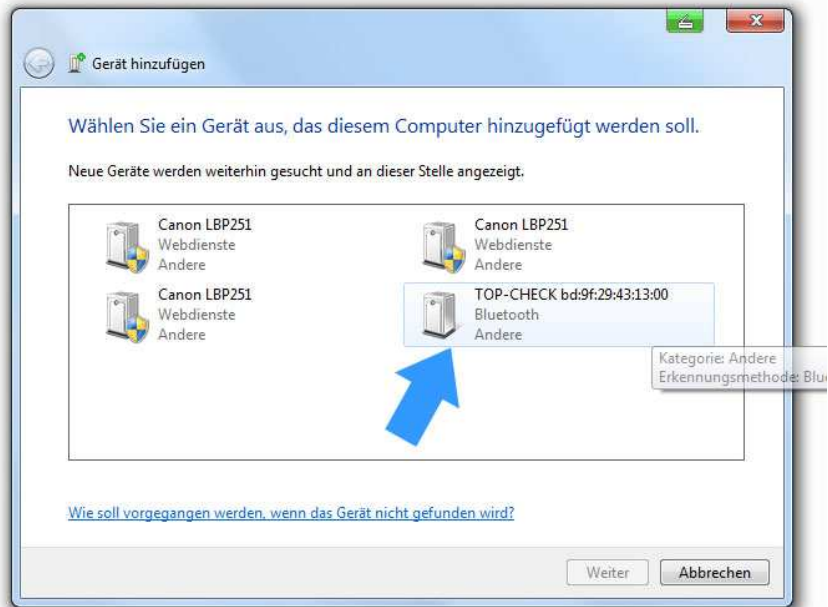

On the PC, the identified TOP-CHECK device must be selected, and the coupling request must be confirmed. An identification number is shown, which you can confirm but ignore.

DETECTING THE COM-PORT

After successful coupling, the TOP-CHECK is assigned to a so-called COM Port. This assignment remains permanent. Before starting the application TOP-CHECK TRANSFER, you must know the number of this port.

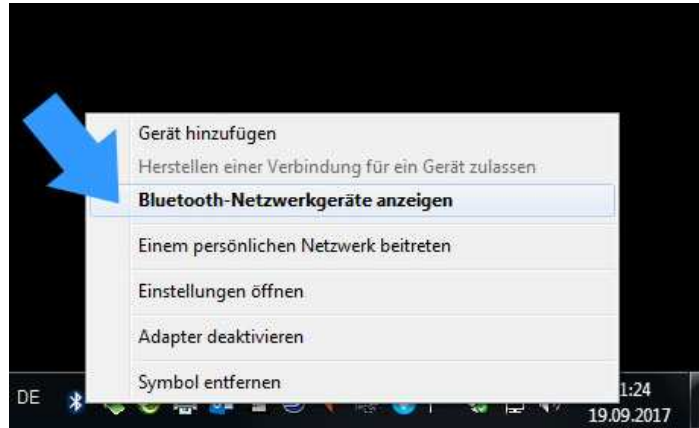

To do this, please determine the assigned COM port number in the Bluetooth device menu. You need to know this at the start of the application TOP-CHECK TRANSFER.

For Windows 10, 2 COM ports are displayed, take the "outbound" number.

Windows 7

The first screenshot shows the Windows 7 'Geräte und Drucker' control panel window. The 'Bluetooth-Geräte' section is active, showing a list of devices. A context menu is open over the device 'TOP-CHECK bd9f29431300', with the 'Eigenschaften' option selected. A blue arrow points to this option.

The second screenshot shows the 'Eigenschaften von TOP-CHECK bd9f29431300' window. The 'Bluetooth' tab is selected, showing a list of services. The 'Serieller Anschluss (SPP) "Serial Port"' service is checked, and its COM port is listed as 'COM23'. A blue arrow points to 'COM23'.

Windows 10

The first screenshot shows the Windows 10 'Einstellungen' app, 'Geräte' > 'Bluetooth' section. The Bluetooth toggle is turned on. A list of devices is shown, with 'TOP-CHECK bd9f29431300' selected. A blue arrow points to this device.

The second screenshot shows the 'Bluetooth-Einstellungen' window for the selected device. It has a tabbed interface with 'COM-Anschlüsse' selected. A table lists the COM ports:

Anschluss	Richtung	Name
COM10	Ausgehend	_TOP-CHECK_2079 "Serial port"
COM11	Ausgehend	TOP-CHECK bd9f29431300 "Serial ..."
COM12	Eingehend	TOP-CHECK bd9f29431300
COM9	Eingehend	TOP-CHECK_2079

A blue arrow points to the 'Ausgehend' direction for COM11.

3. INSTALLING THE APPLICATION


The installation package is called "TOP-CHECK_TRANSFER_Vxx_Setup.exe" (xx = version number) and available for download at

<http://www.list-magnetik.com/de/download>

4. FUNCTIONS


STEP 1: CONNECT

To connect, you need the number of the COM port that you detected in chapter 2. Your TOP-CHECK must be switched on, and Bluetooth must be active in the TOP-CHECK. You can see it: the Bluetooth indicator at the bottom right.

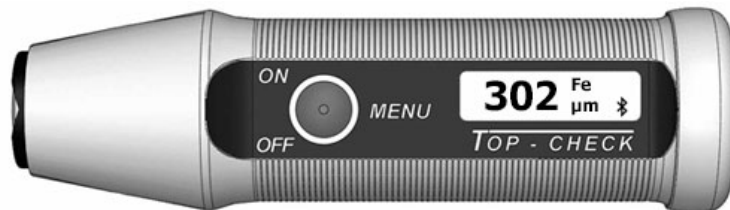


After successful connection, the description changes to "Connected" and the selection box for the COM port becomes invisible. The selected and connected COM port is now shown in the frame headline.

The leftmost of the 3 buttons above the table is displayed with "Online", and the button above is now called "Read first device storage".

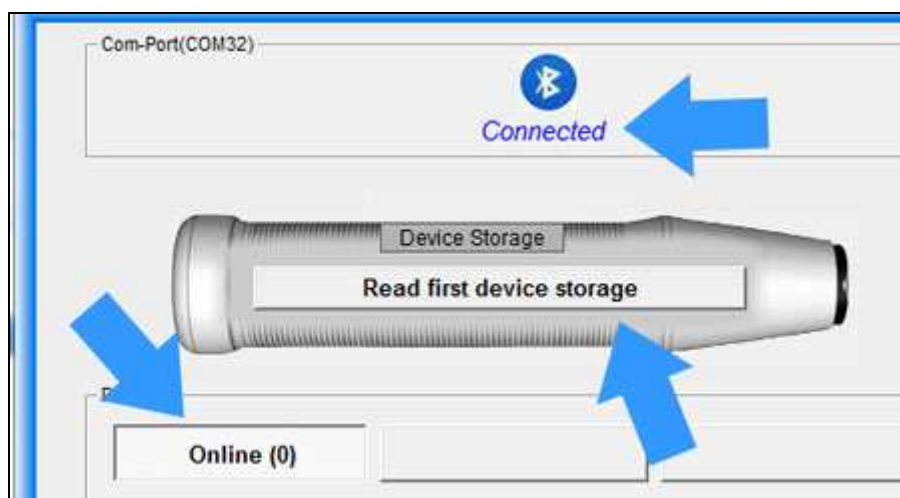


MEASURING ONLINE

Now you can start your work.
For example, you can directly perform online measurements.

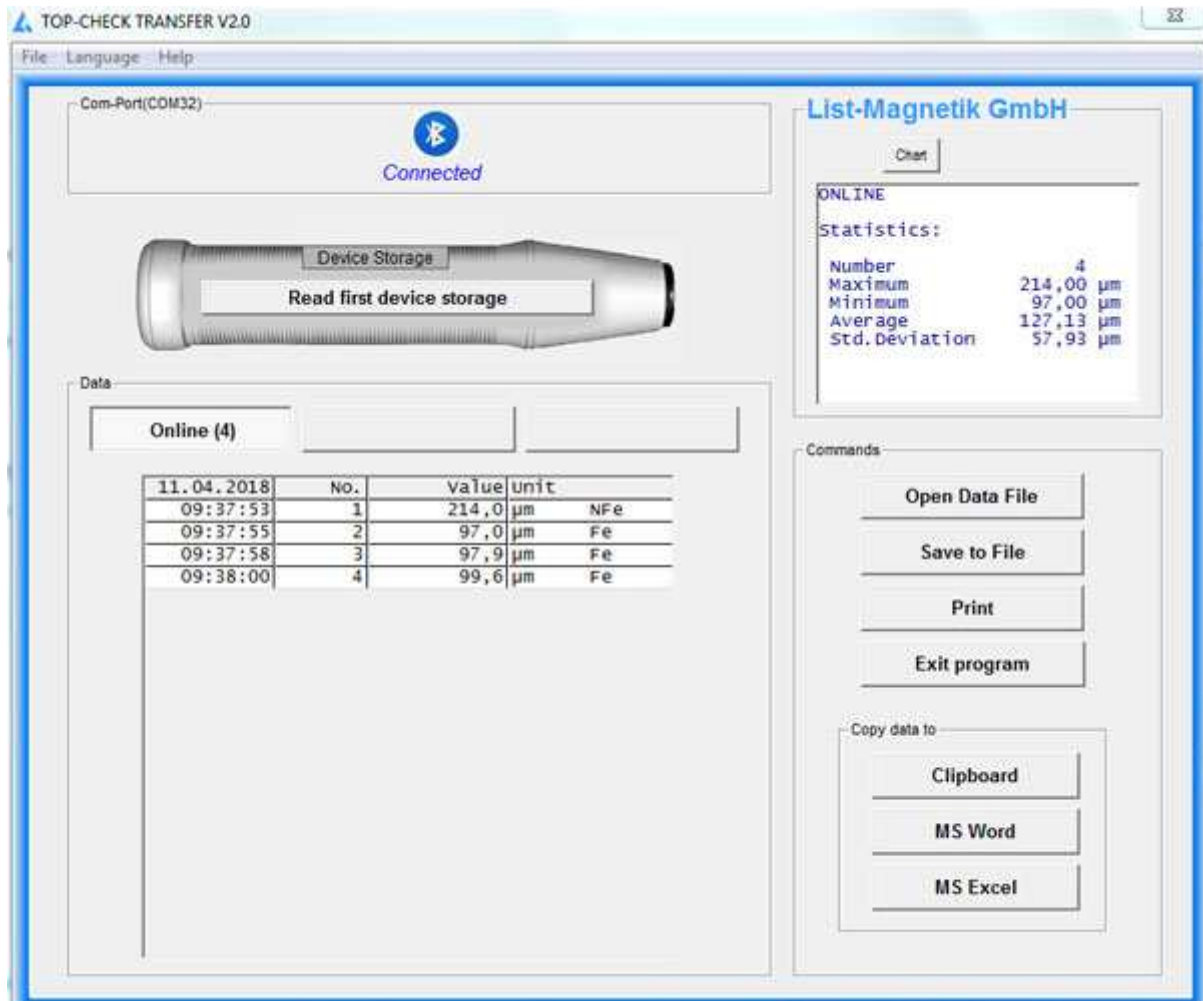

Statistical values are automatically generated from the second measurement: Minimum, Maximum, Average (Mean) and Standard Deviation.


To toggle between the numeric statistic and a line diagram, please use the button "Chart" and "Stat".

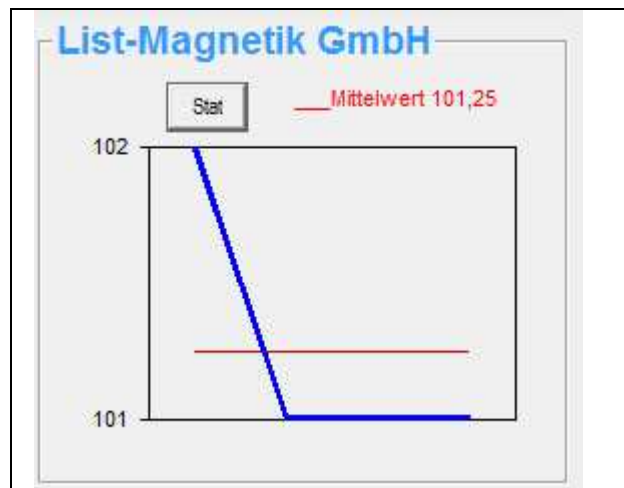


For further processing of the data, see the following sections.

READ DATA FROM DEVICE

If you already have measured values in the device memory, these can be read from the device by the application.

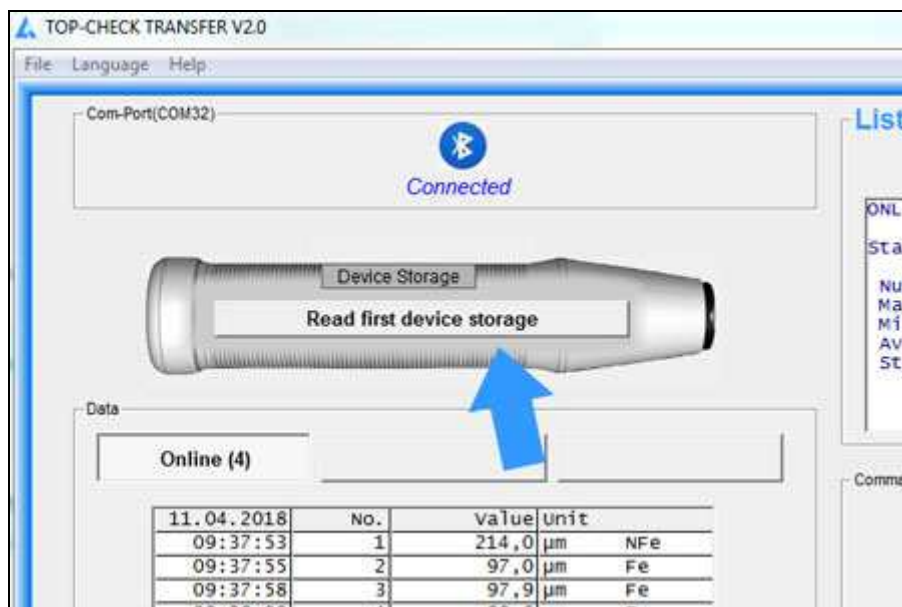

As long as the transfer is running all activities are blocked. The counter behind the title of the measurement series, here "FE-Memory", counts the transferred measurements.

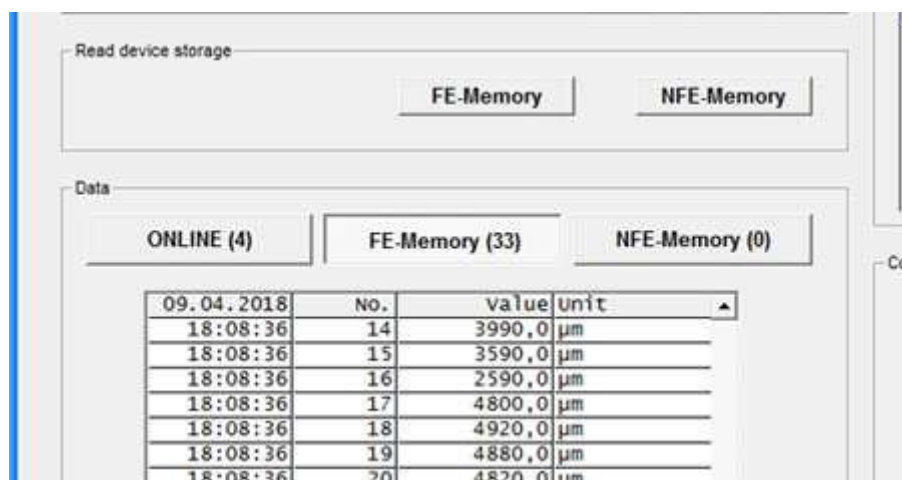


Once the measurement series has been read, the buttons are active again and the statistical data is filled.

As we now know, which type of device you use – either a TOP-CHECK FE-B or a TOP-CHECK FN-B – the buttons now can be filled with the correct terms. A TOP-CHECK FE-B provides a „FE-Memory 1“ and a „FE-Memory 2“, whereas a TOP-CHECK FN-B provides a „FE-Memory“ and a „NFE-Memory“.

OUTPUT: FILE, PRINTER, APPLICATIONS

The measurement series can be stored in a file.
Files of type ".mes" are readable with a text editor.

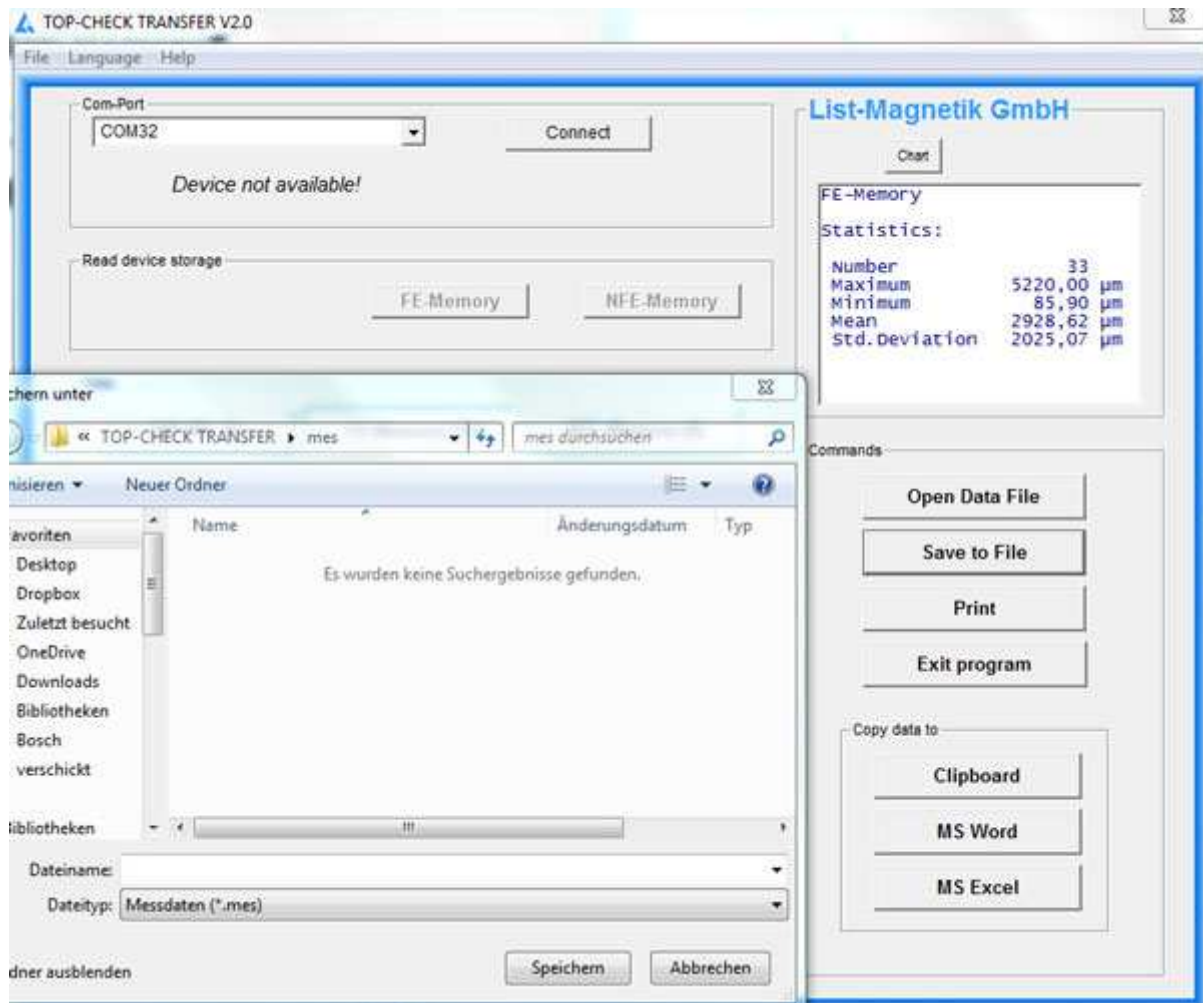


With the button "Open Data File" such a series of measurements can be read again from file, for example to print it or to transfer to Excel.

FE-Memory		
Statistics:		
Number		33
Maximum	5220,00	µm
Minimum	85,90	µm
Mean	2928,62	µm
Std.Deviation	2025,07	µm
09.04.2018		
No.	Value	
18:08:36	1	302,0 µm
18:08:36	2	302,0 µm
18:08:36	3	303,0 µm
18:08:36	4	302,0 µm
18:08:36	5	301,0 µm
18:08:36	6	87,4 µm
18:08:36	7	85,9 µm
18:08:36	8	4230,0 µm
18:08:36	9	4420,0 µm
18:08:36	10	4740,0 µm

Example of a print output via button „Print“

The Buttons „Copy Data to MS Word“ and „Copy Tab to MS Excel“ only will work if the named Microsoft Office components are installed, but not with Open Office.

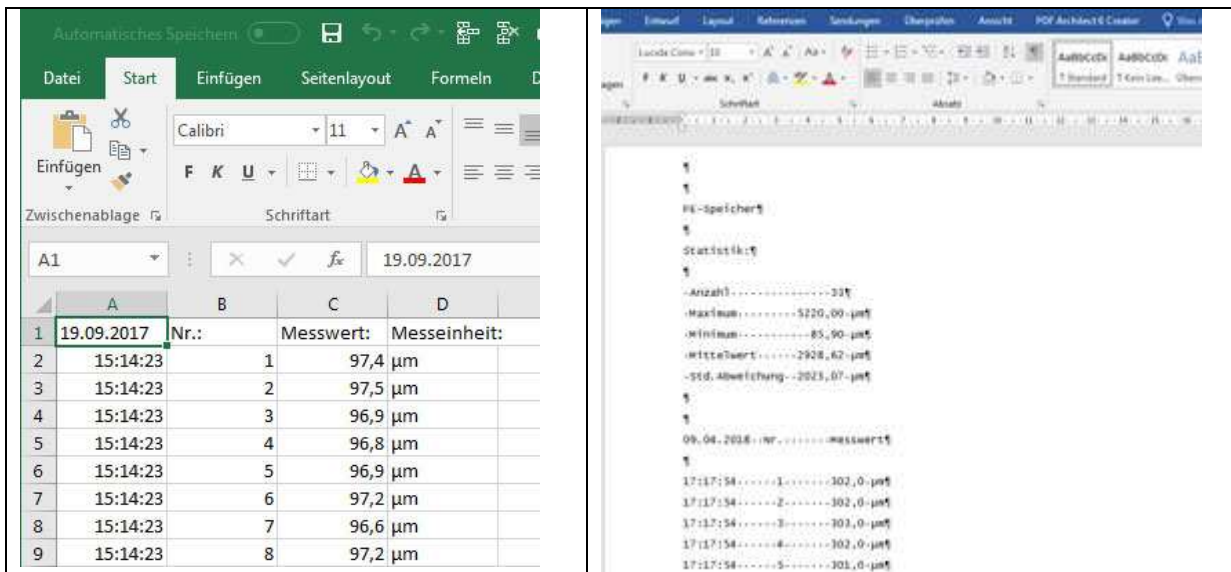

Via Clipboard you can hand over the measuring series to subsequent applications.

OPEN DATA FILE

With then "Open Data File" button you can read in a saved data file again. You must note that the file can only be read in the column from which it was saved (Online measurement series only in Online column, FE only in FE, NFE only in NFE).